

# CRYOPROBES CATALOGUE

## CRYO - S<sup>®</sup> Painless



**A-08/20/N/RF**

REF. number		
N 0 6 0802 2 1		
Tip type	Needle tip with neurostimulation	
Designed for	Cryoanalgesia of the supraorbital, infraorbital, intraoral, auriculotemporal nerve	

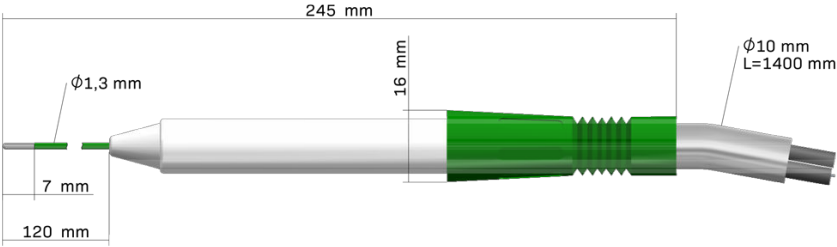
**A-08/90/R/RF**

REF. number		
N 0 6 1312 0 1		
Tip type	Needle tip with neurostimulation	
Designed for	Cryoanalgesia of the supraorbital, infraorbital, intraoral, mental, auriculotemporal nerve	

Green BD catheter included

The expiration date of single use cryoprobes is 3 years

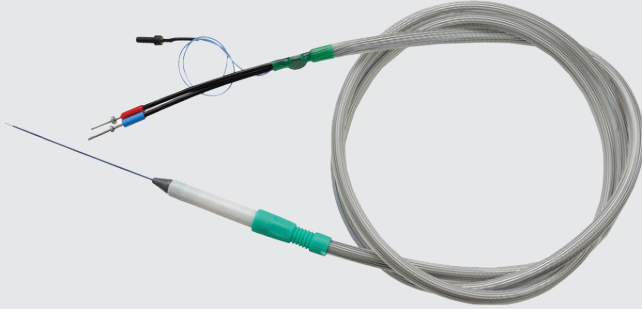

**A-13/120/R/RF**

REF. number	
N 0 6 1312 0 1	
Tip type	
Designed for	

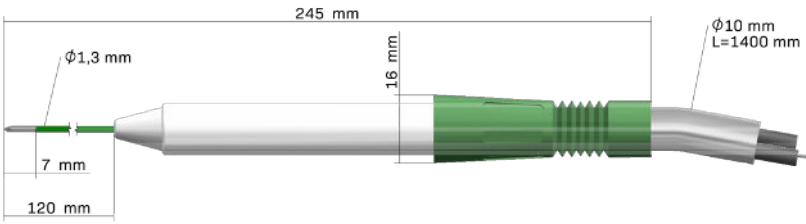
Round tip with neurostimulation

Intercostal nerves, facet joints in the cervical, thoracic, lumbar spine, cryoanalgesia of peripheral nerves and joints denervation

Orange BD catheter included

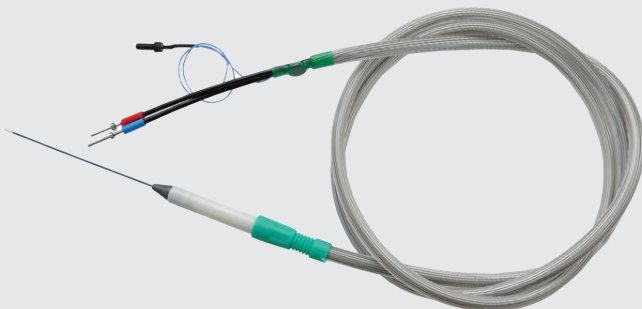

**A-13/120/T/RF**

REF. number	
N 0 6 1312 0 1	
Tip type	
Designed for	

Triangular tip with neurostimulation

Facet joints in the cervical, lumbar spine, cryoanalgesia of peripheral nerves, and joints denervation

Orange BD catheter included

**A-30/PEA/R/RF**


REF. number		
N 0 6 0802 2 1		
Tip type	Round tip without neurostimulation	
Designed for	Cryoanalgesia of intercostal nerve - thoracotomy, VATS	

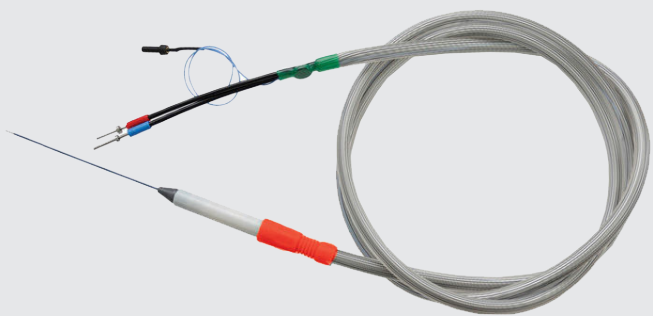
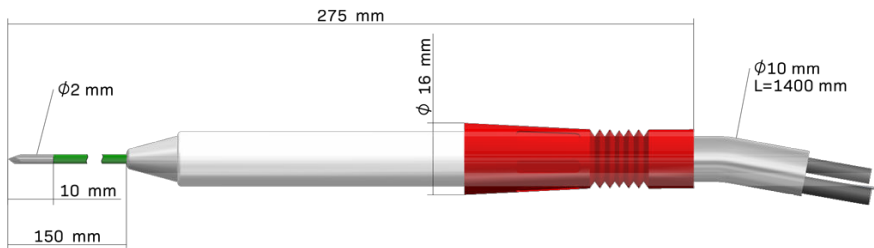
**A-20/SIJ/T/RF**

REF. number		
N 0 6 1312 0 1		
Tip type	Triangular tip without neurostimulation	
Designed for	Cryoanalgesia of sacroiliac joint	

The expiration date of single use cryoprobes is 3 years

**A-20/150/T/RF**

REF. number	
<b>N 0 6 1312 0 1</b>	
Tip type	
 Triangular tip with neurostimulation	
Designed for	
Facet joints in the lumbar, sacral, and iliosacral spine, cryoanalgesia of peripheral nerves, and joints denervation	





# secma

medical innovation

Denmark  
+ 45 8710 1425  
[info@secma.dk](mailto:info@secma.dk)  
[www.secma.dk](http://www.secma.dk)

